



## **T7 RNA Polymerase ELISA Kit**

T7 RNA Polymerase ELISA Kit is an Enzyme Immunoassay kit for the quantification of T7 RNA Polymerase in biopharmaceuticals.

Catalog number: ARG83107

Package: 96 tests

---

For research use only. Not for use in diagnostic procedures.

## **TABLE OF CONTENTS**

<b>SECTION</b>	<b>Page</b>
INTRODUCTION .....	3
PRINCIPLE OF THE ASSAY .....	3
MATERIALS PROVIDED & STORAGE INFORMATION.....	4
MATERIALS REQUIRED BUT NOT PROVIDED.....	4
TECHNICAL NOTES AND PRECAUTIONS .....	5
REAGENT PREPARATION .....	6
ASSAY PROCEDURE .....	8
EXAMPLE OF TYPICAL STANDARD VALUES.....	9
CALCULATION OF RESULTS.....	9

**MANUFACTURED BY:**

Arigo Biolaboratories Corporation

Address: 9F.-7, No. 12, Taiyuan 2nd St., Zhubei City,

Hsinchu County 302082, Taiwan

Phone: +886 (3) 622 1320

Fax: +886 (3) 553 0266

Email: [info@arigobio.com](mailto:info@arigobio.com)

### **INTRODUCTION**

T7 RNA Polymerase ELISA Kit is designed for the quantitative detection of residual T7 RNA Polymerase content added in RNA pharmaceuticals processes by using a double-antibody sandwich method.

### **PRINCIPLE OF THE ASSAY**

T7 RNA Polymerase ELISA kit employs the quantitative sandwich enzyme immunoassay technique. A capture antibody specific for T7 RNA Polymerase has been pre-coated onto a 96 well microplate. T7 RNA Polymerase antigen present in the sample or standard binds to the antibodies adsorbed on the plate; an anti-T7 RNA Polymerase antibody is added and binds to T7 RNA Polymerase. After washing away any unbound substances, a HRP-Conjugate antibody is added and incubation. After washing away any unbound substances, the TMB substrate is added to the wells and color develops in proportion to the amount of DNase I bound in the initial step. The color development is stopped by the addition of stop solution and the intensity of the color is measured at a wavelength of 450 nm. The concentration of DNase I in the samples is then determined by comparing the O.D of samples to the standard curve.

## **MATERIALS PROVIDED & STORAGE INFORMATION**

Use the kit before expiration date.

<b>Component</b>	<b>Quantity</b>	<b>Storage information</b>
Antibody Coated Microplate	8 X 12 strips	4°C
Standard	30 µL (0.668 mg/mL)	-20°C
Sample Diluent Buffer	60 mL (ready to use)	4°C
100X Antibody Conjugate	150 µL	-20°C
Antibody Conjugate Diluent Buffer	12 mL (ready to use)	4°C
100X HRP- Streptavidin Solution	150 µL	-20°C
HRP- Streptavidin Diluent Buffer	12 mL (ready to use)	4°C
20X Wash Buffer	50 mL	4°C
TMB substrate	12 mL (ready to use)	4°C (protect from light)
STOP Solution	7 mL (ready to use)	4°C

## **MATERIALS REQUIRED BUT NOT PROVIDED**

- Microplate reader capable of reading at 450 nm
- Deionized or distilled water
- Pipettes and pipette tips
- Multichannel micropipette reservoir
- Microtiter plate washer


## **TECHNICAL NOTES AND PRECAUTIONS**

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Upon received, store Standard, Antibody Conjugate and HRP at -20°C, store other component at 2-8°C at all times.
- Prior to beginning the assay procedure, bring all reagents and required number of strips to room temperature (20-25°C).
- Unused wells must be stored at 2-8 °C in the sealed foil pouch and used in the frame provided.
- All reagents must be mixed without foaming and briefly spin down the all vials before use.
- If crystals are observed in the 20X Wash Buffer or Diluent Buffer warm to 37°C until the crystals are completely dissolved.
- Minimize lag time between wash steps to ensure the plate does not become completely dry during the assay.
- Ensure complete reconstitution and dilution of reagents prior to use.
- Take care not to contaminate the mixed TMB Substrate. Do not expose the mixed TMB solution to glass, foil or metal. If the solution is blue before use, DO NOT USE IT.
- All reagents must be mixed without foaming before use.
- Change pipette tips between the addition of different reagent or samples.
- Taping the well strips together with lab tape can be done as an extra precaution to avoid plate strips from coming loose during the procedure.

## **REAGENT PREPARATION**

- **1X Wash Buffer:** Dilute **20X Wash Buffer** into **distilled water** to yield **1X Wash Buffer**. The 1X Wash Buffer is stable for up to 4 weeks at 2-8°C. Mix well before use.
- **1X Antibody Conjugate:** It is recommended to prepare this reagent immediately prior to use and use it within 20 min after preparation. Dilute **100X Antibody Conjugate Mixture concentrate** into **Antibody Conjugate Diluent Buffer** to yield 1X Antibody Conjugate.
- **1X HRP-Streptavidin Solution:** It is recommended to prepare this reagent immediately prior to use and use it within 20 min after preparation. Dilute **100X HRP-Streptavidin Solution** into **HRP- Streptavidin Diluent Buffer** to yield 1X HRP-Streptavidin Solution.
- **Standards:** The Diluent Buffer serves as zero standard (0 ng/ml), and the rest of the standard serial dilution can be diluted as according to the suggested concentration below: **256 ng/ml, 128 ng/ml, 64 ng/ml, 32 ng/ml, 16 ng/ml, 8 ng/ml, 4 ng/ml**. DO NOT reuse the reconstituted standard.

## T7 RNA Polymerase ELISA Kit ARG83107

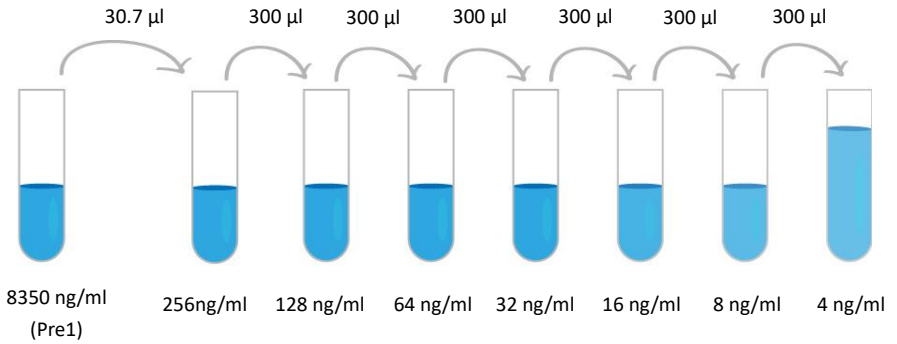

T7 RNA Polymerase standard as according to the table below:

Standard	T7 RNA Polymerase Conc.	µl of Diluent Buffer	µl of standard
<b>Pre 1</b>	<b>8,350 ng/ml</b>	<b>395 µl</b>	<b>5 µl (Stock)</b>
S7	256 ng/ml	969.3 µl	30.7 µl (Pre1)
S6	128 ng/m	300 µl	300 µl(S7)
S5	64 ng/m	300 µl	300 µl(S6)
S4	32 ng/m	300 µl	300 µl(S5)
S3	16 ng/m	300 µl	300 µl(S4)
S2	8 ng/m	300 µl	300 µl(S3)
S1	4 ng/m	300 µl	300 µl(S2)
S0	0 ng/ml	300 µl	0


## **ASSAY PROCEDURE**

All materials should be equilibrated to room temperature (RT, 20-25°C) before use.

1. Add **100 µL** of the **Standard** or **Samples** to the Antibody Coated microplate.
2. Cover the plate and incubate for **1 hours** at **37°C**.
3. Aspirate each well and wash, repeating the process 2 times for a **total 3 washes**. Wash by filling each well with **1X Wash Buffer (350 µL)** using a squirt bottle, manifold dispenser, or autowasher. Keep the wash buffer in the wells for 30-60 sec before remove. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
4. Add **100 µL** of **1X Antibody Conjugate** to each wells.
5. Cover the plate and Incubate for **1 hour** at **37°C**.
6. Aspirate each well and **wash as step 3**.
7. Add **100 µL** of **1X HRP-Streptavidin Solution** to each well.
8. Cover the plate and incubate for **1 hour** at **37°C**.
9. Aspirate each well and **wash as step 3**.
10. Add **100 µL** of **TMB substrate** to each well. Cover and incubate for **10 minutes** at **room temperature** in the dark.
11. Immediately Add **50 µL** of **Stop Solution** to each well, gently tap the plate to mix well. The color of the solution should change from blue to yellow.
12. Read the OD with a microplate reader at **450 nm** immediately. It is recommended reading the absorbance **within 10 minutes** after adding the stop solution.

### **EXAMPLE OF TYPICAL STANDARD VALUES**

The following data is for demonstration only and cannot be used in place of data generations at the time of assay.

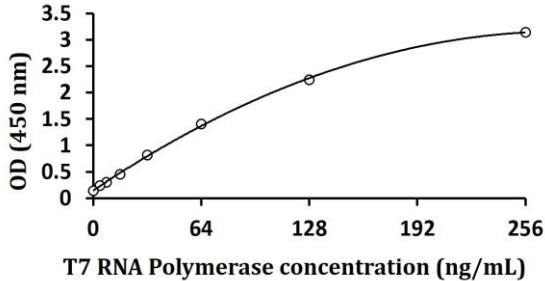

### **CALCULATION OF RESULTS**

1. Calculate the average absorbance values for each set of standards and samples.
2. To obtain more accurate results, more dilution points can be used when generating standard curves. 4 Parameter Logistics is the preferred method for the result calculation. Other data reduction functions may give slightly different results.
3. arigo provides GainData<sup>®</sup>, an in-house development ELISA data calculator, for ELISA data result analysis. Please refer our GainData<sup>®</sup> website for details. (<https://www.arigobio.com/elisa-analysis>)
4. If the samples have been diluted, the concentration read from the standard curve must be further converted by the appropriate dilution factor according to the sample preparation procedure.