



## **Human IL4 ELISA Kit**

Human IL4 ELISA Kit is an Enzyme Immunoassay kit for the quantification of IL4 in Human serum, plasma and cell culture supernatants.

Catalog number: ARG83359

Package: 96 wells

## **TABLE OF CONTENTS**

<b>SECTION</b>	<b>Page</b>
INTRODUCTION .....	3
PRINCIPLE OF THE ASSAY .....	4
MATERIALS PROVIDED & STORAGE INFORMATION .....	5
MATERIALS REQUIRED BUT NOT PROVIDED .....	5
TECHNICAL NOTES AND PRECAUTIONS .....	6
SAMPLE COLLECTION & STORAGE INFORMATION.....	7
REAGENT PREPARATION.....	8
ASSAY PROCEDURE.....	10
CALCULATION OF RESULTS .....	11
EXAMPLE OF TYPICAL STANDARD CURVE .....	12
QUALITY ASSURANCE .....	12

### **MANUFACTURED BY:**

Arigo Biolaboratories Corporation

Address: 9F.-7, No. 12, Taiyuan 2nd St., Zhubei City,

Hsinchu County 302082, Taiwan

Phone: +886 (3) 622 1320

Fax: +886 (3) 553 0266

Email: [info@arigobio.com](mailto:info@arigobio.com)

### INTRODUCTION

The interleukin 4 (IL4, IL-4) is a cytokine that induces differentiation of naive helper T cells (Th0 cells) to Th2 cells. Upon activation by IL-4, Th2 cells subsequently produce additional IL-4 in a positive feedback loop. IL-4 is produced primarily by mast cells, Th2 cells, eosinophils and basophils. It is closely related and has functions similar to IL-13.

Interleukin 4 has many biological roles, including the stimulation of activated B cell and T cell proliferation, and the differentiation of B cells into plasma cells. It is a key regulator in humoral and adaptive immunity. IL-4 induces B cell class switching to IgE, and up-regulates MHC class II production. IL-4 decreases the production of Th1 cells, macrophages, IFN $\gamma$ , and dendritic cells IL-12. IL-4 signaling determines the levels of CD20 on the surface of normal and malignant B lymphocytes via activation of transcription factor STAT6.

Overproduction of IL-4 is associated with allergies.

### PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for Human IL4 has been pre-coated onto a microtiter plate. Standards or samples are pipetted into the wells and any IL4 present is bound by the immobilized antibody. After washing away any unbound substances, a biotin-conjugated antibody specific for Human IL4 is added to each well and incubate. Following a washing to remove unbound substances, streptavidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. After washing away any unbound antibody-enzyme reagent, a TMB Substrate is added to the wells and color develops in proportion to the amount of Human IL4 bound in the initial step. The color development is stopped by the addition of acid and the intensity of the color is measured at a wavelength of  $450\text{nm} \pm 2\text{nm}$ . The concentration of Human IL4 in the sample is then determined by comparing the O.D of samples to the standard curve.

### MATERIALS PROVIDED & STORAGE INFORMATION

Store 100X Antibody Conjugate at -20°C and other components at 2-8°C. Use the kit before expiration date.

Component	Quantity	Storage information
Antibody Coated Microplate	8 x 12 strips	4°C.
Standard	3 X 0.5 ng/vial	4°C
Standard / Sample Diluent Buffer	20 mL (Ready to use)	4°C
100X Antibody Conjugate	120 µL	-20°C
100X HRP-Streptavidin	120 µL	4°C
Antibody Diluent Buffer	30 mL (Ready to use)	4°C
20X Wash Buffer	45 mL	4°C
TMB Substrate	12 mL (Ready to use)	4°C (Protect from light)
STOP Solution	12 mL (Ready to use)	4°C
Plate Sealers	3 strips	Room temperature

### MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of reading at O.D. 450 nm
- Centrifuge and centrifuge tube
- Deionized or Distilled water
- Pipettes, pipette tips and Multichannel micropipette reservoir
- Automated microplate washer (optional)

### TECHNICAL NOTES AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Upon received, store 100X Antibody Conjugate at -20°C. Store other components at 2-8°C at all times.
- Prior to beginning the assay procedure, bring all reagents and required number of strips to room temperature.
- Briefly spin down the all vials before use.
- If crystals are observed in the 20X Wash Buffer, warm to 37°C until the crystals are completely dissolved.
- Minimize lag time between wash steps to ensure the plate does not become completely dry during the assay.
- Ensure complete reconstitution and dilution of reagents prior to use.
- Take care not to contaminate the TMB Substrate. Do not expose the TMB Substrate to glass, foil or metal. Do NOT return leftover TMB Substrate to bottle. Do NOT contaminate the unused TMB Substrate. If TMB Substrate is blue before use, DO NOT USE IT.
- Change pipette tips between the addition of different reagent or samples.
- Taping the well strips together with lab tape can be done as an extra precaution to avoid plate strips from coming loose during the procedure.
- Include a standard curve each time the assay is performed.
- Run both standards and samples in at least duplicates.

## **SAMPLE COLLECTION & STORAGE INFORMATION**

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

**Cell Culture Supernatants** - Remove particulates by centrifugation for 10 min at 1500 x g at 4°C and aliquot & store samples at -20°C up to 1 month or -80°C up to 6 months. Avoid repeated freeze-thaw cycles.

**Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Collect serum and assay immediately or aliquot & store samples at -20°C up to 1 month or -80°C up to 6 months. Avoid repeated freeze-thaw cycles.

**Plasma** - Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge for 15 minutes at 1000 x g. within 15 min of collection. Collect the supernatants and assay immediately or aliquot and store samples at -20°C up to 1 month or -80°C up to 6 months. Avoid repeated freeze-thaw cycles.

### **Note:**

- Do not use haemolytic, icteric or lipaemic specimens.
- Samples containing sodium azide should not be used in the assay.

### REAGENT PREPARATION

- **1X Wash Buffer:** Dilute **20X** Wash Buffer into 1X distilled water to yield 1X Wash Buffer (E.g., add 25 mL of 10X Wash Buffer into 475 mL of distilled water to a final volume of 500 mL).

The diluted 1X Wash Buffer is stable for 4 weeks at 2°C to 8°C.

- **1X Antibody Conjugate:** 20 minutes before use, dilute **100X** Antibody Conjugate into **Antibody Diluent Buffer** to yield 1X Antibody Conjugate.
- **1X HRP-Streptavidin:** 20 minutes before use, dilute **100X** HRP-Streptavidin into **Antibody Diluent Buffer** to yield 1X HRP-Streptavidin. Keep diluted HRP-Streptavidin in dark before use.
- **Sample:** If initial assay results indicate that sample concentrations exceed the highest point of the standard curve, dilute the samples using the provided **Standard / Sample Diluent Buffer** and re-assay.

A preliminary experiment is recommended for all sample types to determine the optimal dilution factor. For serum and plasma samples, a 1:1 dilution with the **Standard / Sample Diluent Buffer** (dilution factor = 2) is generally sufficient in most cases.

Note: When calculating final concentrations, be sure to apply the appropriate dilution factor.



## Human IL4 ELISA Kit ARG83359

---

- **Standard:** Centrifuge the un-reconstituted standard at 6000 x g for 1 minute to bring down the material prior to open the vial. Add **1 ml** of **Standard / Sample Diluent Buffer** to a Standard vial to make the high standard concentration of 500 pg/mL and brief vortex for few seconds (Do not induce foaming) and allow it to sit at room temperature for 15 minutes. Make sure the standard is dissolved completely before making serial dilutions. The Standard / Sample Diluent Buffer serves as zero standard (0 pg/ml), and the rest of the standard serial dilution can be diluted with Standard / Sample Diluent Buffer. Diluted the standard as below:

Standard tube	IL4 (pg/mL)	Standard / Sample Diluent Buffer (μL)	Standard (μL)
S1	500	0	1000 (500 pg/mL Standard Stock)
S2	250	500	500 of S1
S3	125	500	500 of S2
S4	62.5	500	500 of S3
S5	31.25	500	500 of S4
S6	15.63	500	500 of S5
S7	7.81	500	500 of S6
S0	0	500	0

**Note:** Working standard should be prepared immediately prior to use.

### ASSAY PROCEDURE

All materials should be equilibrated to room temperature (RT, 20-25°C) before use. Standards and samples should be assayed in duplicates.

1. Add **100 µL** of **diluted samples** or **each diluted Standard** into respective wells of the 96-well plate.
2. Cover the plate and incubate for **2 hour** at **room temperature**.
3. Aspirate each well and wash, repeating the process 4 time for a **total 5 washes**. Wash by filling each well with **1X Wash Buffer (300 µL)** using a squirt bottle, manifold dispenser, or auto-washer. Keep the Wash Buffer in the wells for 60 sec before remove. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
4. Add **100 µL** of **1X Antibody Conjugate** to each well.
5. Cover the plate and incubate for **1 hour** at **room temperature**.
6. Aspirate each well and **wash plate as step 3**.
7. Add **100 µL** of **1X HRP-Streptavidin** to each well.
8. Cover the plate and incubate for **1 hour** at **room temperature** in the dark.
9. Aspirate each well and **wash plate as step 3**.
10. Add **100 µL** of **TMB Substrate** in each well.
11. Incubate for **10-15 min** at **room temperature** in the dark.
12. Add **100 µL** of **STOP Solution** to each well to stop the reaction.
13. Read the absorbance with a plate reader at **O.D. 450 nm**. It is recommended reading the absorbance within 15 min after adding the STOP Solution.

### CALCULATION OF RESULTS


1. Calculate the average absorbance values for each set of standards, control and samples.
2. Using log-log, semi-log or linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.
3. Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
4. Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
5. arigo provides GainData®, an in-house development ELISA data calculator, for ELISA data result analysis. Please refer our GainData® website for details. (<https://www.arigobio.com/elisa-analysis>)
6. If the samples have been diluted, the concentration read from the standard curve must be further converted by the appropriate dilution factor according to the sample preparation procedure as described above.

## Human IL4 ELISA Kit ARG83359

---

### EXAMPLE OF TYPICAL STANDARD CURVE

The following figures demonstrate typical results with the Human IL4 ELISA Kit. One should use the data below for demonstration only and cannot be used in place of data generations at the time of assay.

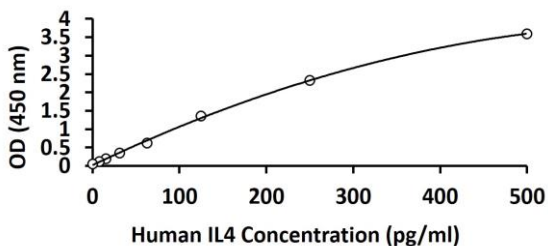

### QUALITY ASSURANCE

#### Sensitivity

3.9 pg/ml

#### Assay Range

7.8- 500 pg/ml