



Human Ferritin ELISA Kit

Enzyme Immunoassay for the quantification of Ferritin in human serum and plasma

Catalog number: ARG80501

Package: 96 wells

For research use only. Not for use in diagnostic procedures.

TABLE OF CONTENTS

SECTION	Page
INTRODUCTION.....	3
PRINCIPLE OF THE ASSAY	4
MATERIALS PROVIDED & STORAGE INFORMATION	5
MATERIALS REQUIRED BUT NOT PROVIDED.....	6
TECHNICAL HINTS AND PRECAUTIONS	6
SAMPLE COLLECTION & STORAGE INFORMATION.....	7
REAGENT PREPARATION.....	8
ASSAY PROCEDURE.....	8
CALCULATION OF RESULTS	9
EXAMPLE OF TYPICAL STANDARD CURVE	10
QUALITY ASSURANCE	11

MANUFACTURED BY:

Arigo Biolaboratories Corporation

Address: 9F.-7, No. 12, Taiyuan 2nd St., Zhubei City,

Hsinchu County 302082, Taiwan

Phone: +886 (3) 622 1320

Fax: +886 (3) 553 0266

Email: info@arigobio.com

INTRODUCTION

Ferritin is a globular protein found mainly in the liver, which can store about 2'250 iron (Fe^{3+}) ions. The ferritin molecule consists of a protein shell (apoferritin) composed of heavy and light subunits, which surrounds a crystalline core containing iron oxide and phosphate.

Ferritin is synthesized in the liver, spleen and numerous other body tissues, with major concentrations found in the liver, spleen, bone marrow, and intestinal mucosa

The ferritin levels measured have a direct correlation with the total amount of iron stored in the body. If ferritin is high there is iron in excess, which would be excreted in the stool. If ferritin is low there is a risk for lack in iron, which sooner or later could lead to anemia.

In the setting of anemia, serum ferritin is the most sensitive lab test for iron deficiency anemia. In contrast, serum ferritin levels are normal or increased in anemia associated with chronic disease. Elevated serum ferritin levels have been observed in acute and chronic liver disease and lymphoid malignancy (leukemia and Hodgkin lymphoma). High serum ferritin levels have also been associated with an elevated risk for myocardial infarction in men. Ferritin is also used as a marker for iron overload disorders, such as haemochromatosis in which the ferritin level may be abnormally raised.

Human Ferritin ELISA Kit ARG80501

Ferritin is an acute-phase reactant, it is often elevated in the course of disease.

Free iron is toxic to cells, and the body has an elaborate set of protective mechanisms to bind iron in various tissue compartments. Within cells, iron is stored complexed to protein as ferritin or hemosiderin. Apoferritin binds to free ferrous iron and stores it in the ferric state. Under steady state conditions, the serum ferritin level correlates with total body iron stores; thus, the serum ferritin level is the most convenient laboratory test to estimate iron stores.

PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for Ferritin has been pre-coated onto a microtiter plate. Standards or samples are pipetted into the wells and any Ferritin present is bound by the immobilized antibody. After washing away any unbound substances, an HRP conjugated antibody specific for Ferritin is added to each well and incubate. A substrate solution (TMB) is then added to the wells and color develops in proportion to the amount of Ferritin bound in the initial step. The color development is stopped by the addition of acid and the intensity of the color is measured at a wavelength of 450 nm \pm 2 nm. The concentration of Ferritin in the sample is then determined by comparing the O.D of samples to the standard curve.

Human Ferritin ELISA Kit ARG80501

MATERIALS PROVIDED & STORAGE INFORMATION

Store the unopened kit at 2-8 °C. Use the kit before expiration date

Component	Quantity	Storage information
Antibody-coated microplate	1 plate	4°C
Standard 1-5 (5, 20, 100, 400, 800 ng/ml)	5 X 1 ml (Ready-to-use)	4°C
Zero Standard	3 ml (Ready-to-use)	4°C
Control (78.3 ng/ml; acc. range: 55.2-102 ng/ml)	1 ml (Ready-to-use)	4°C
HRP-Conjugated antibody	21 ml (Ready-to-use)	4°C
10X Wash buffer	50 ml	4°C
TMB substrate	15 ml (Ready-to-use)	4°C (Protect from light)
STOP solution	15 ml (Ready-to-use)	4°C

MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of measuring absorbance at 450nm (optional: read at 620-630 nm as the reference wave length)
- Pipettes and pipette tips
- Deionized or distilled water
- Automated microplate washer (optional)

TECHNICAL HINTS AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Store the kit at 4°C in the dark at all times. Do not expose reagents to heat, sun, or strong light during storage and usage.
- Open the bag of antibody-coated microplate only when it is at room temperature and close it immediately after use, once opened, it is stable until the expiry date of the kit. Do not remove the adhesive sheets on the strips unutilized.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C. We recommend consumption on the same day.
- Briefly spin down the antibody conjugate concentrate and HRP-Streptavidin concentrate before use.
- All materials must be at room temperature (20-28°C) prior to use.
- If crystals are observed in the 50X Wash buffer, warm to RT or 37°C until the crystals are completely dissolved.
- Ensure complete reconstitution and dilution of reagents prior to use.

Human Ferritin ELISA Kit ARG80501

- It is highly recommended that the standards, samples and controls be assayed in duplicates.
- All incubation steps must be accurately timed.
- Change pipette tips between the addition of different reagent or samples.

SAMPLE COLLECTION & STORAGE INFORMATION

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

Serum- Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20 °C. Avoid repeated freeze-thaw cycles.

Plasma- Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20 °C. Avoid repeated freeze-thaw cycles.

Note:

- a) Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- b) Samples containing sodium azide should not be used in the assay.
- c) Testing of heat-inactivated sera is not recommended.

REAGENT PREPARATION

- **1X Wash buffer:** Dilute 10X Wash buffer into distilled water to yield 1X Wash buffer. (E.g. 50 ml of 10X Wash buffer + 450 ml of distilled water.) Diluted wash buffer is stable for 30 days at 2-8°C.
- **Sample:** If the initial assay found samples contain Ferritin higher than the highest standard, the samples can be diluted with Zero Standard and then reassay the samples. For the calculation of the concentrations this dilution factor has to be taken into account. The sample must be well mixed with the diluents buffer before assay.
Store the sample at -20°C if the determination is not performed on the same day of the sample collection. Before using, mix gently, for 5 minutes, with a roller mixer.
- **HRP-Conjugated antibody:** The HRP-Conjugated antibody is ready to use. Mix gently, for 5 minutes, on a roller mixer.

ASSAY PROCEDURE

All materials should be equilibrated to room temperature (RT, 22-28°C) for at least 30 min. All reagents should be store at 2 °C- 8 °C immediately after used and avoid long exposure to room temperature. Standards, samples and controls should be assayed in duplicates.

1. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal it and stored at 2°C - 8°C.
2. Add **10 µl** of **standards, controls and samples** in duplicate into wells. Keep

Human Ferritin ELISA Kit ARG80501

one well empty as blank.

3. Add **200 µl** of **HRP-conjugated antibody** into each well, except blank well. Gently tap the plate to mix well. **Incubate for 1 hours at RT.**
4. Aspirate each well and wash, repeating the process 2 times for a **total 3 washes**. Wash by filling each well with **1× Wash Buffer (300 µl)** using a squirt bottle, manifold dispenser, or autowasher. Gently shake the plate for 5 seconds. Then complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
Note: if you use automated equipment, wash the wells at least 5 times.
5. Add **100 µl** of **TMB Substrate Reagent** to each well (including blank well). Incubate for **15 minutes at room temperature in dark.**
6. Add **100 µl** of **Stop Solution** to each well. Shake the microplate gently. The color of the solution should change from blue to yellow.
7. **Read** the OD with a microplate reader **at 450 nm** against a reference wavelength of 620-630 nm or against Blank. It is recommended read the absorbance within 5 minutes after adding stop solution.

CALCULATION OF RESULTS


1. Calculate the average absorbance values for each set of standards, controls and patient samples.
2. Using semi-log or linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.

Human Ferritin ELISA Kit ARG80501

- Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
- Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
- If the samples have been diluted, the concentration read from the standard curve must be further converted by the appropriate dilution factor according to the sample preparation procedure as described above.

EXAMPLE OF TYPICAL STANDARD CURVE

The following data is for demonstration only and cannot be used in place of data generations at the time of assay.

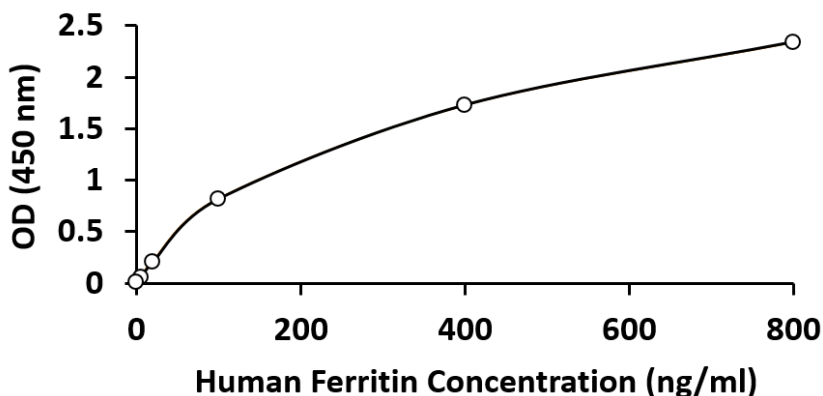

QUALITY ASSURANCE

Sensitivity

The minimum detectable dose (MDD) of Ferritin ranged from 2.84-800 ng/ml.

The mean MDD was 2 ng /ml.

Intra-assay and Inter-assay precision

The CV value of intra-assay precision was <7.5 % and inter-assay precision was < 6.1.

Specificity

The following substances do not interfere with a bias of > ±15% in the Ferritin ELISA when the concentrations are below the stated threshold presented in the following table.

Potentially Interfering Reagent	Threshold Concentration
Bilirubin, conjugated	15 mg/dL
Bilirubin, unconjugated	15 mg/dL
Haemoglobin	1000 mg/dL
Total Protein	10 g/dL
Triglyceride	3000 mg/dL

Recovery

95.76-107.43%